

**Yocom-McColl Testing Laboratories, Inc.**  
 540 West Elk Place • Denver, Colorado 80216-1823 USA  
 PHONE (303) 294-0582 • FAX (303) 295-6944  
 EMAIL: ymccoll@ymccoll.com

**Optical Fiber Diameter Analyser (OFDA100)  
 Micron Test Report**

Lodi Alpacas/Jan Clingman  
 W12002 Slack Road  
 Lodi WI 53555 USA

06/24/10

Test No: 379776


**Animal and Sample Description**

**Animal Name:** SSR Bellisio  
**Breed:** Alpaca(Suri)  
**Sex:** Male  
**Color:** Light Fawn

**Animal ID:** 30992696  
**Sample Location:** Side  
**Sample Date:** 05/09/10  
**Age:** 04/26/08

**Laboratory Data**

<b>Mean Fiber Diameter:</b>	21.2 microns	<b>Spin Fineness:</b>	20.4 microns
<b>Standard Deviation:</b>	4.2 microns	<b>Mean Curvature (deg/mm):</b>	11.6
<b>Coefficient of Variation:</b>	19.6 %	<b>SD Curvature (deg/mm):</b>	12.5
<b>Fibers Greater Than 30 microns:</b>	2.2 %	<b>Comfort Factor:</b>	97.8 %
<b>Medullated Fibers:</b>	10.0 %		

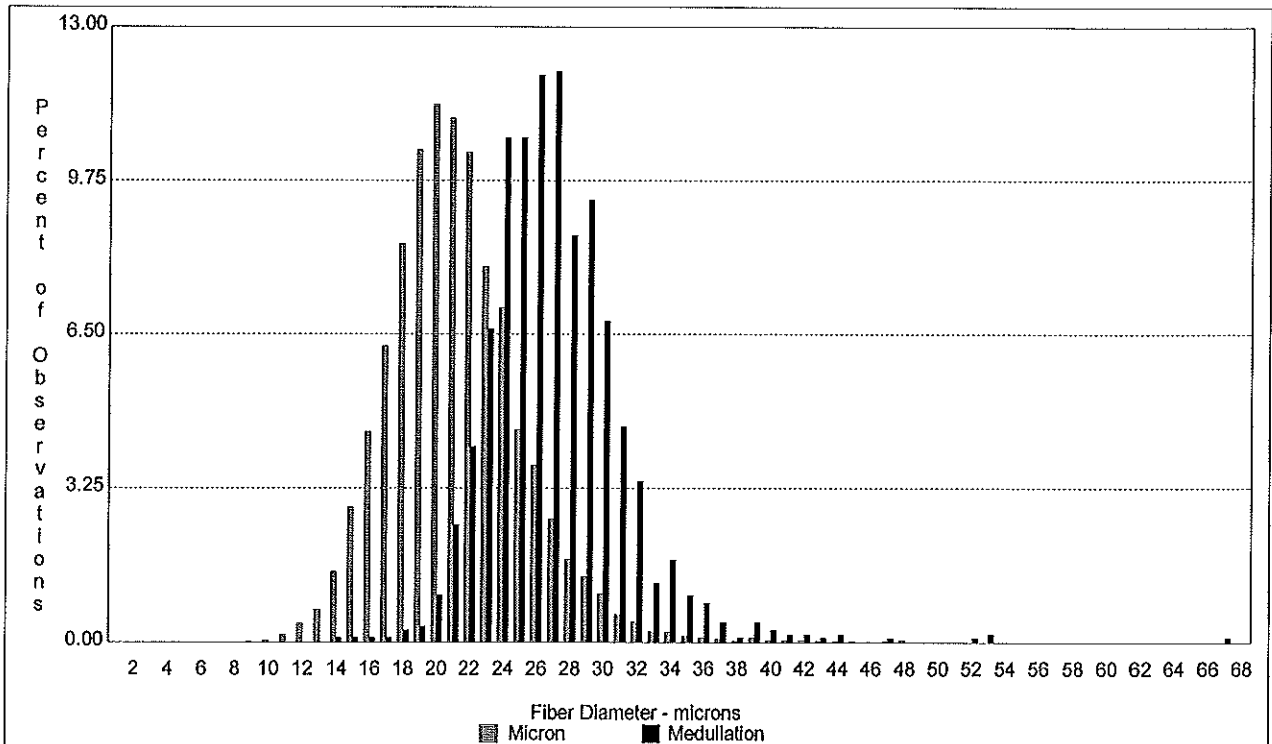

**This Test Performed According to I.W.T.O Method 47**