



Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

**Optical Fiber Diameter Analyser (OFDA100)
Micron Test Report**

Lodi Alpacas/Jan Clingman
W12002 Slack Road
Lodi WI 53555 USA

06/24/10

Test No: 379778


Animal and Sample Description

Animal Name: SSR Alakef
Breed: Alpaca(Suri)
Sex: Male
Color: Dark Fawn

Animal ID: 1098600
Sample Location: Side
Sample Date: 05/09/10
Age: 10/18/05

Laboratory Data

Mean Fiber Diameter:	30.6 microns	SpIn Fineness:	30.5 microns
Standard Deviation:	7.3 microns	Mean Curvature (deg/mm):	8.1
Coefficient of Variation:	23.8 %	SD Curvature (deg/mm):	11.4
Fibers Greater Than 30 microns:	39.8 %	Comfort Factor:	60.2 %

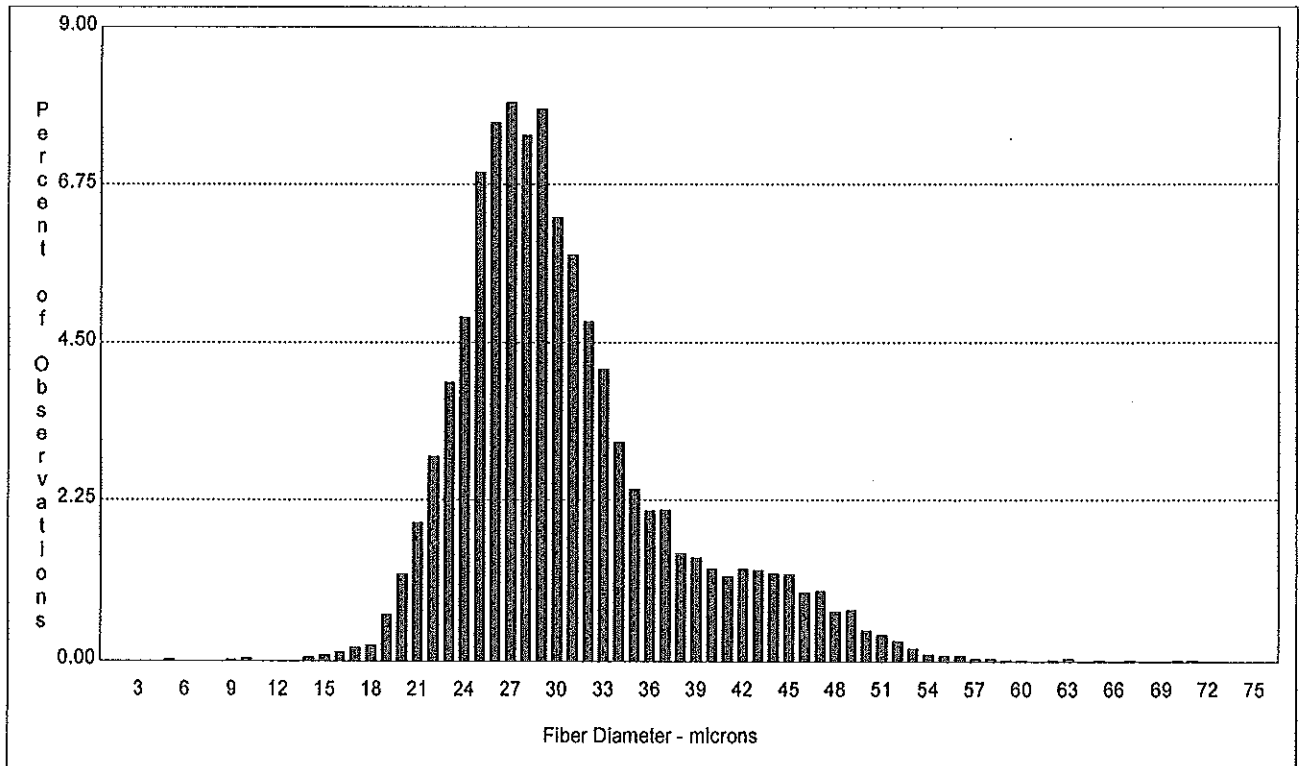

This Test Performed According to I.W.T.O Method 47